



BS-230

Clinical Chemistry Analyzer



FusionGreen Healthcare Pvt. Ltd.

We deliver ...

mindray

healthcare within reach



Flexible loading:

Up to 80 sample ports

Up to 80 reagent ports

(40 x red + 40 interchangeable)


100µl

minimum reaction volume




FusionGreen Healthcare Pvt. Ltd.

We deliver...

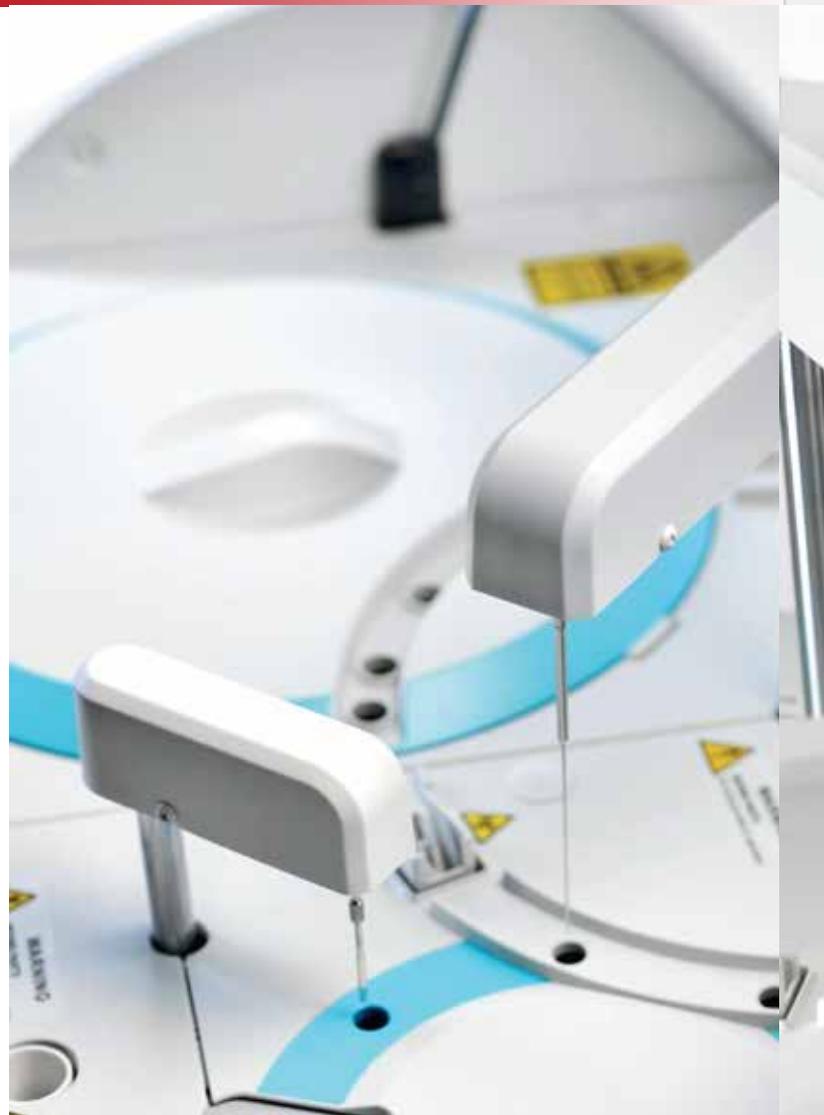

Disposable Cuvettes

to avoid contamination

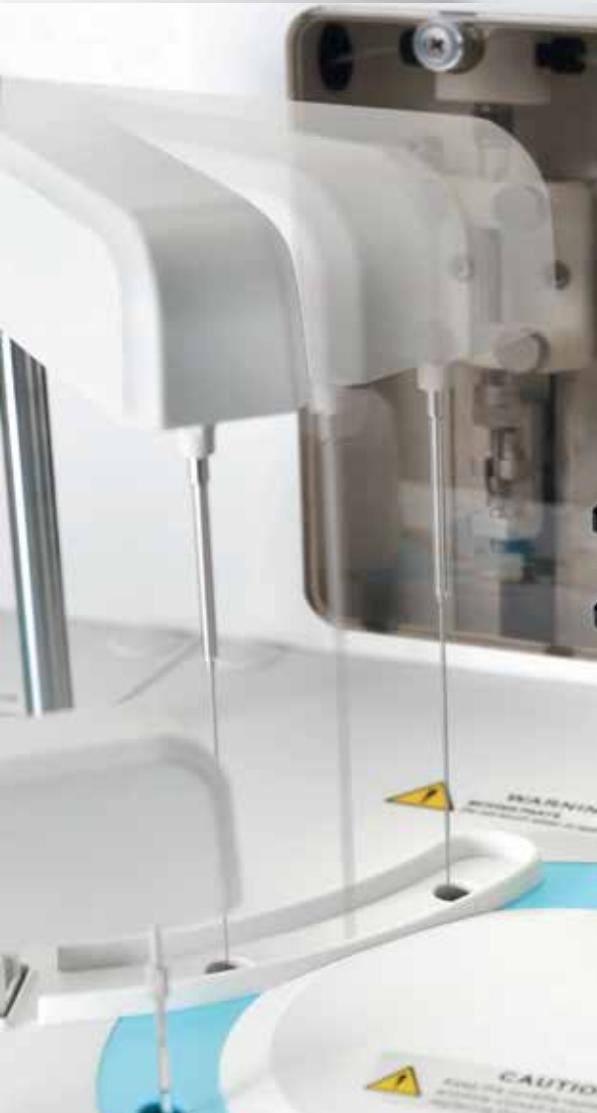

Probe carryover less than

0.05%



FusionGreen Healthcare Pvt. Ltd.

We deliver ...



BS-230

Clinical Chemistry Analyzer



Independent mixing bar



Built-in barcode reader



Intelligent software with user-friendly interface



Step-by-step maintenance guide





FusionGreen Healthcare Pvt. Ltd.

We deliver...


Compact Size with Robust Functions



Complete traceability process

Complete calibration hierarchy and traceability chain are based on ISO standard (EN/ISO17511) from reference system to routine measurement system.

Traceability chain of Mindray measurement system (Glu)

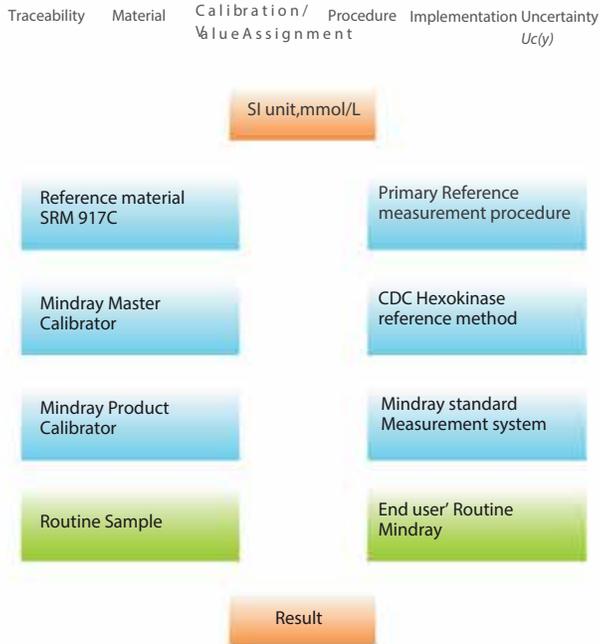


External quality assurance for reference measurement

Mindray participates in RELA (External quality control for reference laboratory) and CAP (College of American Pathologists external quality control).

EQA for Mindray Reference laboratory——RELA

Mindray reference laboratory has passed RELA for 6 consecutive years.

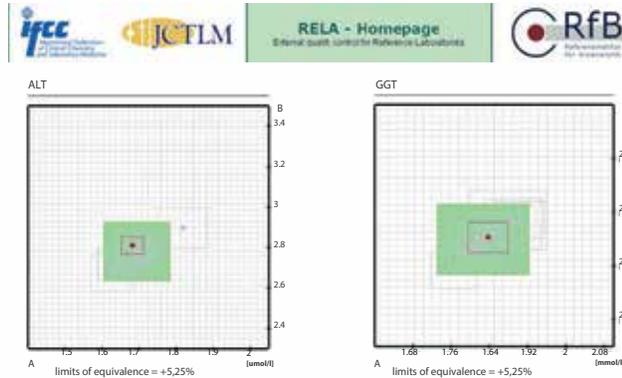

More RELA results please refer to: www.dgkl-rfb.de/81




All the items Mindray participate RELA

ALT AMY ALP CK GGT GLU LDH TB TP UA UREA

EQA for Mindray Testing System——CAP

Mindray testing system has passed CAP for 6 consecutive years.



CAP Number: 7198395-01 Kit#1
Institution: Shenzhen Mindray Biomed Elec Co Ltd
Attention: Lixing Liu MD
City / State: Hongkong HK CH 518055

Kit ID: 25733824
Kit Mailed: 6/3/2013
Original Evaluation: 7/8/2013

EVALUATION
ORIGINAL

C-B 2013 Chemistry

CAP

Regulated Analyte	Proficiency Event 2012		Proficiency Event 2013		Proficiency Event 2013		Current Event Performance Interpretation	Cumulative CLIA '88 Performance Interpretation
	Test Event	Score %	Test Event	Score %	Test Event	Score %		
ALT	C-C C-C C-	5/ 100	C-A	5/5 100	C-B C-B C-B	5/5 100	Satisfactor	Successful
Albumin	C-C C-C C-	5/ 100	C-A	5/5 100	C-B C-B C-B	5/5 100	y	Successful
Alkaline Phosphatase	C-C C-C C-	5/ 100	C-A	5/5 100	C-B C-B C-B	5/5 100	Satisfactor	Successful
Amylase	C C-C C-C	5/ 100	C-A	5/5 100	C-B C-B C-B	5/5 100	y	Successful
AST	C-C C-C C-	5/ 100	C-A	5/5 100	C-B C-B C-B	5/5 100	Satisfactor	Successful
Bilirubin, Total	C C-C C-C	5/ 100	C-A	5/5 100	C-B C-B C-B	5/5 100	y	Successful
Calcium, Total	C-C C-C C-	5/ 100	C-A	5/5 100	C-B C-B C-B	5/5 100	Satisfactor	Successful
Chloride	C C-C C-C	5/ 100	C-A	5/5 100	C-B	5/5 100	y	Successful
Cholesterol, Total	C-C C-C	5/ 100	C-A	5/5 100	C-B	5/5 100	Satisfactor	Successful
Cholesterol, HDL		5/ 100	C-A	5/5 100		5/5 100	y	Successful
Creatine Kinase	5/ 100		C-A	5/5 100		5/5 100	Satisfactor	Successful
Cr eatinine	5/ 100		C-A	5/5 100		5/5 100	y	Successful
Glucose	5/ 100		C-A	5/5 100		5/5 100	Satisfactor	Successful
Iron, Total	5/ 100		C-A	5/5 100		5/5 100	y	Successful
LD	5/ 100		C-A	5/5 100		5/5 100	Satisfactor	Successful
Magnesium	5/ 100		C-A	5/5 100		5/5 100	y	Successful
Potassium	5/ 100		C-A	5/5 100		5/5 100	Satisfactor	Successful
Sodium	5/ 100		C-A	5/5 100		5/5 100	y	Successful
Protein, Total	5/ 100		C-A	5/5 100		5/5 100	Satisfactor	Successful
Triglycerides	5/ 100		C-A	5/5 100		5/5 100	y	Successful
Urea Nitrogen	5/ 100		C-A	5/5 100		5/5 100	Satisfactor	Successful
Uric Acid	5/ 100		C-A	5/5 100		5/5 100	y	Successful
	5/						Satisfactor	
	5/						y	
	5/						Satisfactor	
	5/						y	
	5/						Satisfactor	
	5/						y	

Reagent menu

Hepatic Panel

Alanine Aminotransferase (ALT)
 Aspartate Aminotransferase (AST)
 Alkaline Phosphatase (ALP)
 γ -GlutamylTransferase (γ -GT)
 Direct Bilirubin (D-Bil) DSA Method
 Direct Bilirubin (D-Bil)VOX Method
 Total Bilirubin (T-Bil) DSA Method
 Total Bilirubin (T-Bil)VOX Method
 Total Protein (TP)
 Albumin (ALB)
 Total Bile Acids (TBA)
 Prealbumin (PA)
 Cholinesterase (CHE)
 α -L-fucosidase (AFU)
 5'-nucleotidase (5'-NT)

Renal Panel

Urea (UREA)
Creatinine (CREA) Modified Jaffé Method
 Creatinine (CREA)Sarcosine Oxidase Method
 Uric Acid (UA)
 Carbon dioxide (CO₂)
 Microalbumin
 β 2-Microglobulin (β 2-MG)
 Cystatin C (CysC)
 Retinol binding protein(RBP)

Immune Panel

Immunoglobulin A (IgA)
 Immunoglobulin G (IgG)
 Immunoglobulin M (IgM)
 Complement C3 (C3)
 Complement C4 (C4)

Diabetes Panel

Glucose (Glu) GOD-POD Method
 Glucose (Glu) HK Method
 Hemoglobin A1c (HbA1c)
 Fructosamine (FUN)
 β -Hydroxybutyrate(β -HB)

Cardiac panel

Creatine Kinase (CK)
 Creatine Kinase-MB (CK-MB)
 Lactate Dehydrogenase (LDH)
 α -Hydroxybutyrate Dehydrogenase(α -HBDH)
 High sensitive C-reaction protein(HS-CRP)

Inorganic & Anemia

Iron (Fe)
 Ferritin (FER)
 Transferrin (TRF)
 Calcium (Ca)
 Magnesium (Mg)
 Phosphate Inorganic (P)
 Unsaturated iron binding capacity (UIBC)
 Glucose-6-phosphate dehydrogenase (G6PD)

Lipid Panel

Total Cholesterol (TC)
 Triglycerides (TG)
 HDL-Cholesterol (HDL-C)
 LDL-Cholesterol (LDL-C)
 Apolipoprotein A1 (ApoA1)
 Apolipoprotein B (ApoB)
 Lipoprotein(a) [Lp(a)]

Rheumatism Panel

C-reactive protein (CRP)
 Rheumatoid Factor (RF)
 Antibodies Against Streptolysin O (ASO)

Lung Panel

Adenosine Deaminase (ADA)
 Angiotensin Converting Enzyme(ACE)

Pancreatitis Panel

α -Amylase (α -AMY)
 Lipase (LIP)



BS-230

ClinicalChemistry Analyzer

Technical Specifications

System function

Automatic, Discrete, Random Access, Bench-top

STAT sample priority

Throughput: Up to 200 tests/hour, up to 400 tests/hour with ISE

Measuring principles: Absorbance photometry, Turbidimetry, Ion Selective Electrode technology

Methodology: End-point, Fixed-time, Kinetic, optional ISE, Single/Dual/ reagent chemistries, monochromatic / bi-chromatic

Original system pack reagent ready to use

Close system and open system is optional

Reagent/Sample Handling

Reagent/Sample tray: 80 positions for reagents and 40 positions for samples in 24-hour refrigerated compartment (2~12°C)

Reagent volume: 10~250µl, step by 0.5µl

Sample volume: 2~45µl, step by 0.1µl

Reagent/Sample probe: Liquid level detection, vertical collision protection and inventory checking, reagent pre-warming

Probe cleaning: Automatic washing for interior and exterior Carry over < 0.05%

Automatic sample dilution: Pre-dilution and post-dilution

Internal bar code reader (optional)

Capable to communicate with LIS in bi-directional mode

Reaction System:

Cuvette: 40 disposable cuvettes

Reaction volume: 100~360µl

Operating temperature: 37°C±0.1 °C

ISE Module (optional)

Measuring K+, Na+, Cl-

Mixing Unit

Independent mixing bar

Optical System

Light Source: Halogen-tungsten lamp

Wavelength: 8 wavelengths, 340nm、405nm、450nm、510nm、546nm、578nm、630nm、670nm

Absorptionrange:0~4.0 Abs (10mm conversion), resolution 0.0001Abs

Stray Light 5.6Abs

Control and Calibration

Calibration modes: Linear (one point, two points and multi-points), Logit-Log 4P, Logit-Log 5P, spline, exponential, polynomial, parabola

Control Rules: X-R, L-J, Westgard multi-rule, Cumulative sum check, twin plot

Operation Unit

Operation system: Windows 8

Interface: RS-232

Working Conditions

Power Supply: 200~240V, 50/60Hz, ≤1000VA or 100~130V, 60Hz, ≤1000VA

Dimension: 690 mm (length) ×580 mm (depth) ×595 mm (height)

Weight: 47 kg

Water Consumption: ≤ 2 L/H



Marketed By:



+91 9677144414, 9940141956

TOLL FREE NO: 1800-203-2528

Corporate Office: FusionGreen Healthcare Pvt Ltd

7, East Chetty Street, Ramapuram, Ravi Colony, Gandhi Nagar, St.Thomas Mount, Chennai, Tamil Nadu 600016.

Customer Relations & Training Center:

FusionGreen Healthcare Pvt Ltd - "Krishna" Ground Floor No 51/6, First Link Street, Raghavan Colony, Ashok Nagar, Chennai - 600 083, Tamil Nadu, India.

Branch Offices: Coimbatore & Madurai

Mindray Building, Keji 12th Road South,
High-tech Industrial Park, Nanshan, Shenzhen 518057, P.R. China
Tel: +86 755 8188 8998 Fax: +86 755 26582680
E-mail: intl-market@mindray.com www.mindray.com

mindray are registered trademarks or trademarks owned by Shenzhen Mindray Bio-medical Electronics Co., LTD.
©2015ShenzhenMindrayBio-MedicalElectronics Co., Ltd. All rights reserved.Specifications subject to changes without prior notice.
P/N: ENG-BS-230-21285x8-20160314

mindray